




Simple, Reliable Qualitative QC Microorganisms

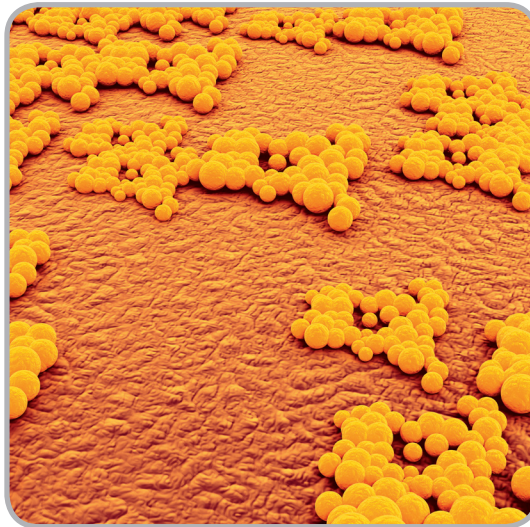

Applications:

- Culture purposes
- Daily QC
- Verification and validation
- QC of identification systems and assay kits
- QC of Antimicrobial Susceptibility Test

Product Details:


- User-friendly design with a lyophilized microorganism pellet, ampoule of hydrating fluid and inoculating swab
- Packs of two or six
- Also available in QC Sets and Panels. Each set or panel is designed to contain the recommended quality control strains for a particular test method, assay or regulatory standard.

Highlights:

- Extensive, diverse collection of strains available
- All-in-one design reduces the risk of contamination
- Ready-to-use format saves you time and money
- Online Certificate of Analysis provides detailed strain information
- Traceability to reference cultures ensures authenticity
- Technical Support experts available for guidance


How to Use KWIK-STIK™

1

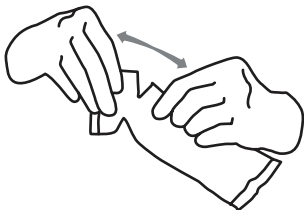

Allow the unopened KWIK-STIK™ pouch to equilibrate to room temperature. Tear open pouch at notch and remove the KWIK-STIK unit.

2

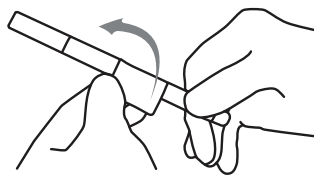


Tear off pull-tab portion on the label and attach it to the primary culture plate or QC record. Do not disassemble the device during hydration.

3

Over the edge of the work bench or counter, crack the ampoule at the top of the KWIK-STIK (just below the fluid meniscus of the ampoule) found in the cap to release the hydrating fluid.

4

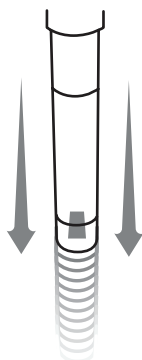

Hold vertically and tap on a hard surface to facilitate flow of the fluid through the shaft into the bottom of unit where the pellet is contained.

5




Using a pinching action on the bottom portion of the unit, crush the pellet in the fluid until the pellet suspension is homogenous.

6




Immediately heavily saturate the swab with the hydrated material and transfer to the appropriate agar medium, or use according to the laboratory's SOP.

7

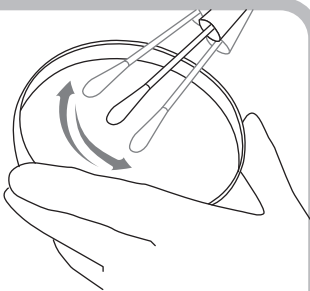

Inoculate the primary culture plate(s) by gently rolling the swab over one-third of the plate.

8

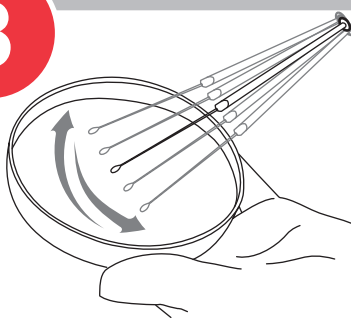

Using a sterile loop, streak to facilitate colony isolation.

9

Using proper biohazard disposal, discard the KWIK-STIK.



10

Immediately incubate the inverted inoculated primary culture plate(s) at temperature and conditions appropriate to the microorganism.

Culture method can be found on the product's page at microbiologics.com